

File D:\DATA\T91\MONITOR\CP-0006590-091-00112-LCMSA033.D

Injection Date : 19 Mar 12 4:32 pm +0800

Tgt Mass (EZX) : 217.00

Sample Name : CP-0006590-091

Location : P1-A-07

Acq. Operator : T91-Monitor

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 0.5 ul

Acq. Method : D:\METHODS\1-POS-MON-3MIN.M

Analysis Method : D:\METHODS\1-POS-MON-3MIN.M

Sample Info : 217.00

Method Info : Column: SunFire C18, 4.6x50mm, 3.5um


Mobile phase: H2O(0.05%TFA) (A) / ACN(0.05%TFA) (B)

Elution program: Gradient from 5 to 95% of B in 1.2min at 2ml/min


Temperature: 50 °C

Detection: UV (214 , 4 nm) and MS (ESI, Pos mode , 70 to 1000 amu)


*ADC1 A, ELSD

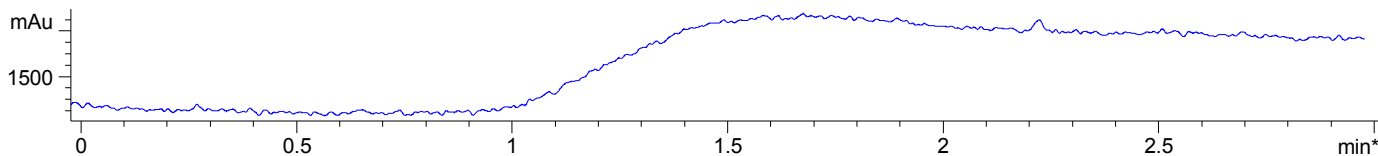


*DAD1 A, Sig=214,4 Ref=off

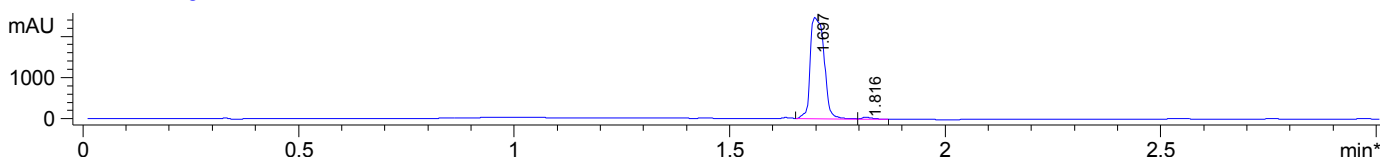


*DAD1 B, Sig=254,4 Ref=off

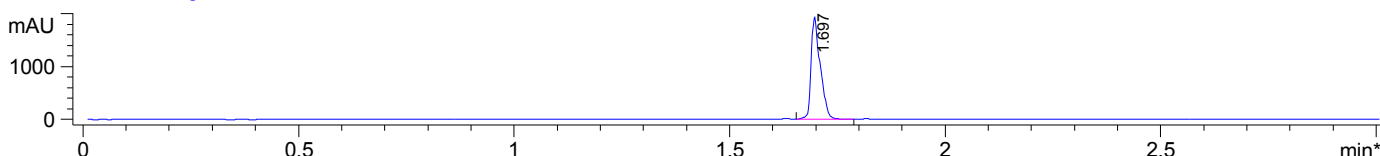

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

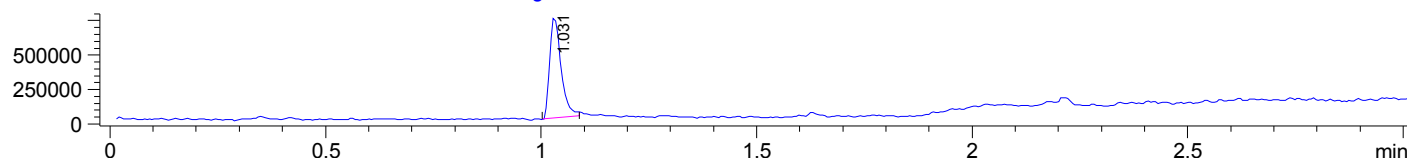

Ion 218, MSD1 218, Target Mass 217 +H Positive, EIC=217.7:218.7

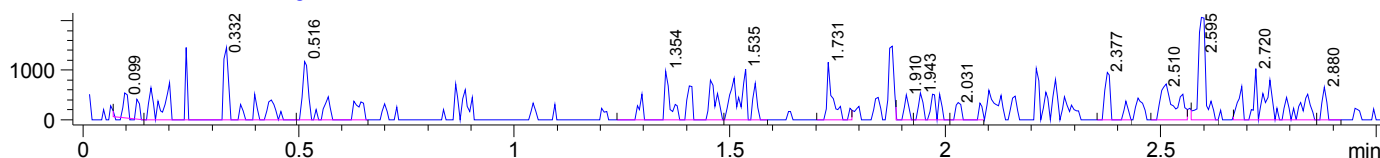

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
--------	-------	------	--------	-------

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.70	0.03	5514.43	2451.88	98.65
1.82	0.02	75.30	52.24	1.35

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.70	0.02	2899.45	1927.50	100.00

Ret. Time: 1.03

<<<< POSITIVE SPECTRA >>>>

