



File D:\DATA\T91\MONITOR\CP-0006590-090-4-00089-LCMSA033.D

Injection Date : 19 Mar 12 2:46 pm +0800 Tgt Mass (EZX) : 146.00
Sample Name : CP-0006590-090-4 Location : P1-F-04
Acq. Operator : T91-Monitor Inj : 1
Spec. Reported : MS Integration Inj Volume : 2 ul
Acq. Method : D:\METHODS\1-POS-MON-3MIN.M
Analysis Method : D:\METHODS\1-POS-MON-3MIN.M
Sample Info : 146.00
Method Info : Column: SunFire C18, 4.6x50mm, 3.5um
Mobile phase: H2O(0.05%TFA) (A) / ACN(0.05%TFA) (B)
Elution program: Gradient from 5 to 95% of B in 1.2min at 2ml/min
Temperature: 50 °C
Detection: UV (214 , 4 nm) and MS (ESI, Pos mode , 70 to 1000 amu)


*ADC1 A, ELSD

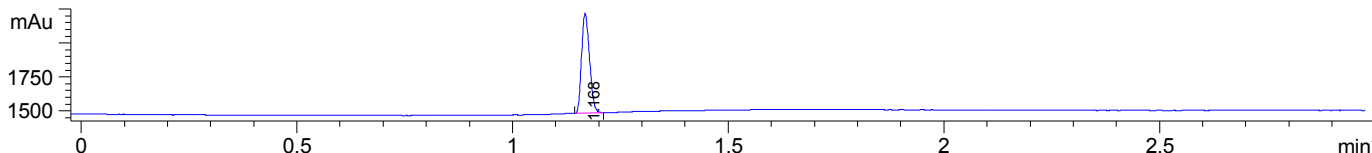


*DAD1 A, Sig=214,4 Ref=off

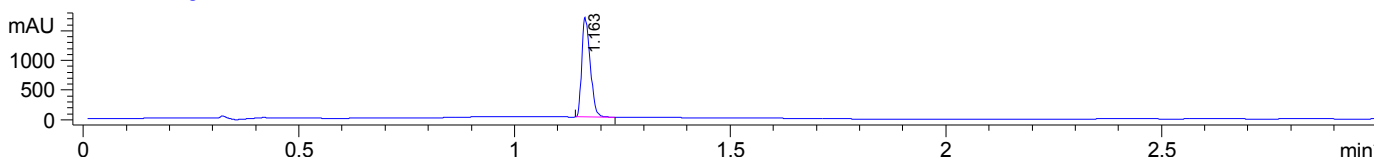


*DAD1 B, Sig=254,4 Ref=off

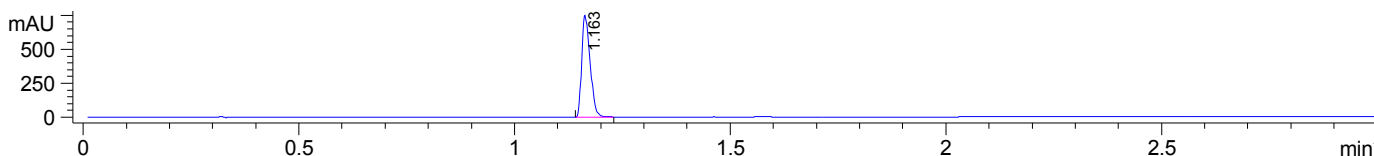

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

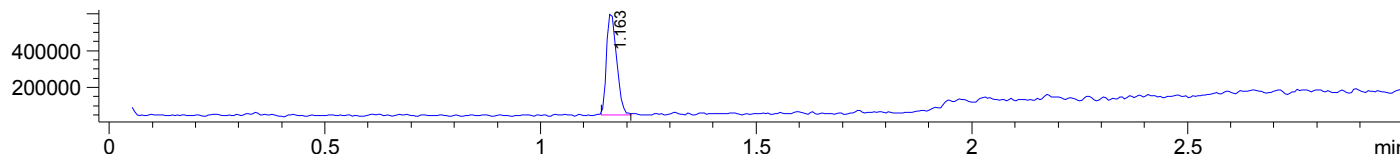

Ion 147, MSD1 147, Target Mass 146 +H Positive, EIC=146.7:147.7

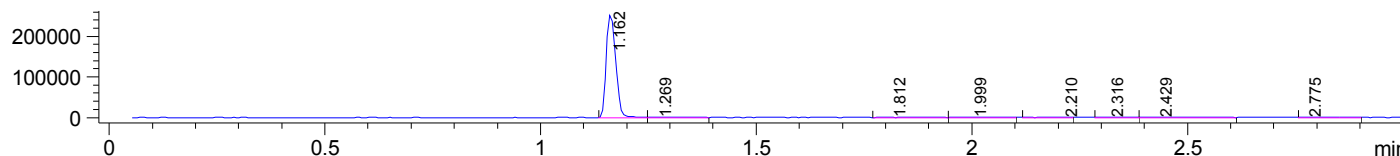

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
1.17	0.02	938.36	732.28	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.16	0.02	2283.14	1675.28	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.16	0.02	1010.27	747.29	100.00

Ret. Time: 1.16

<<<< POSITIVE SPECTRA >>>>

