

File D:\DATA\T91\MONITOR\CP-0006590-105-1-00481-LCMSA033.D

Injection Date : 22 Mar 12 1:40 pm +0800 Tgt Mass (EZX) : 212.00

Sample Name : CP-0006590-105-1

Location : P2-A-03

Acq. Operator : T91-Monitor

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 1 ul

Acq. Method : D:\METHODS\1-POS-MON-3MIN.M

Analysis Method : D:\METHODS\1-POS-MON-3MIN.M

Sample Info : 212.00

Method Info : Column: SunFire C18, 4.6x50mm, 3.5um


Mobile phase: H2O(0.05%TFA) (A) / ACN(0.05%TFA) (B)

Elution program: Gradient from 5 to 95% of B in 1.2min at 2ml/min


Temperature: 50 °C

Detection: UV (214 , 4 nm) and MS (ESI, Pos mode ,70 to 1000 amu)


*ADC1 A, ELSD

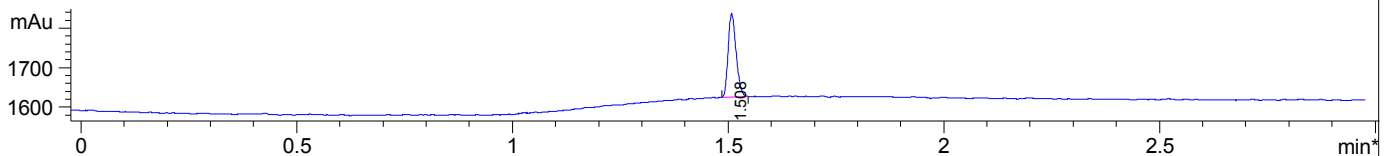


*DAD1 A, Sig=214,4 Ref=off

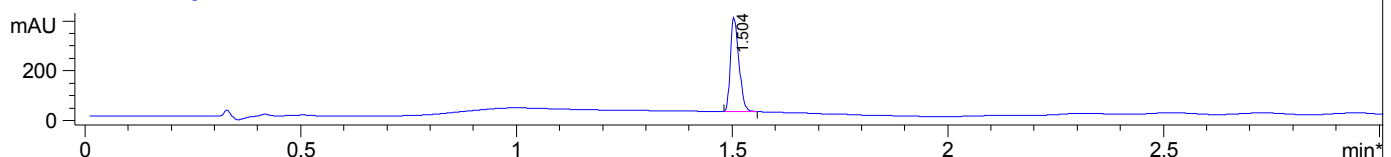


*DAD1 B, Sig=254,4 Ref=off

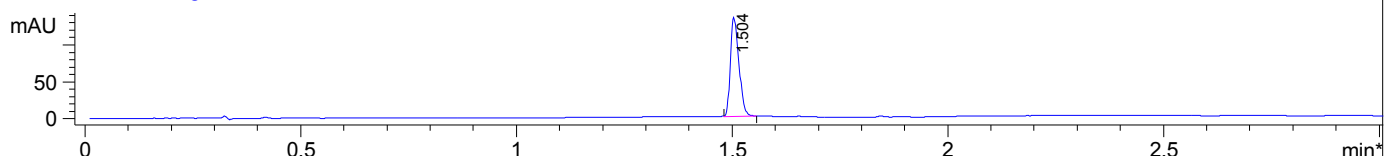

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

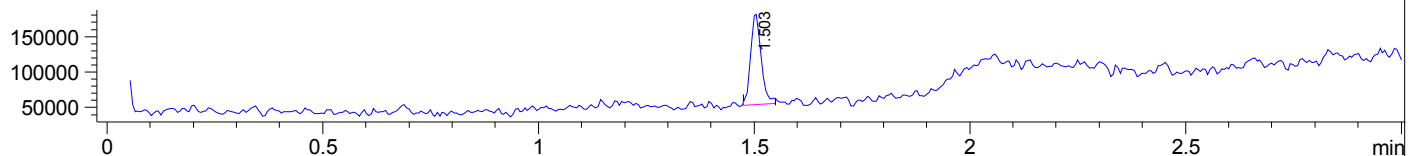

Ion 213, MSD1 213, Target Mass 212 +H Positive, EIC=212.7:213.7

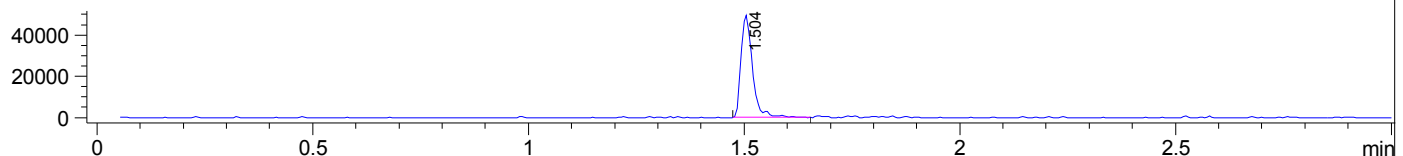

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
1.51	0.02	273.19	211.71	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.50	0.02	522.24	376.99	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.50	0.02	185.49	133.57	100.00

Ret. Time: 1.50

<<<< POSITIVE SPECTRA >>>>

